
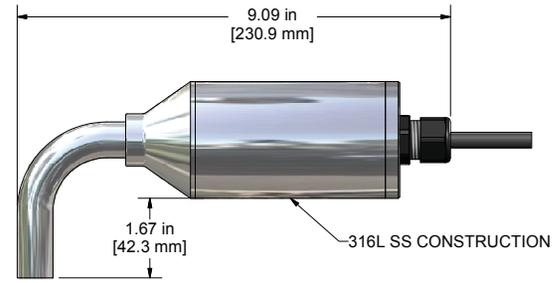
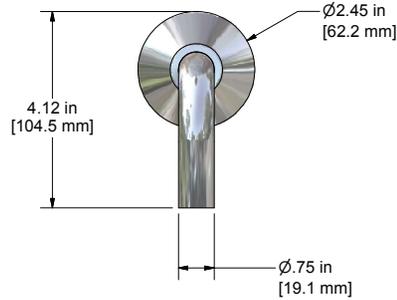





## DIRECT MOUNT 12" FIBER OPTIC BUNDLE MOUNT

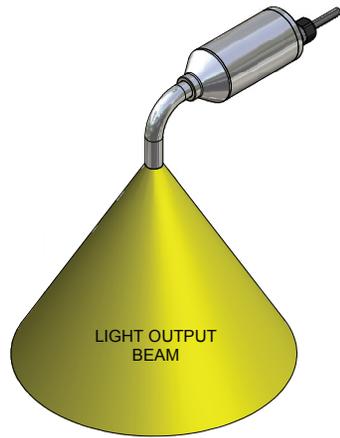

SIDE

MOUNT DIRECT TO SIGHT GLASS USING CANTY OR CUSTOMER SUPPLIED BRACKET. RIGID FIBER OPTIC BUNDLE SUPPORTS LIGHT. SEE DATASHEET TD10811-200 FOR OPTIONAL MOUNTING BRACKET OPTIONS.

## REMOTE MOUNT 24" + LONGER FIBER OPTIC BUNDLE MOUNT

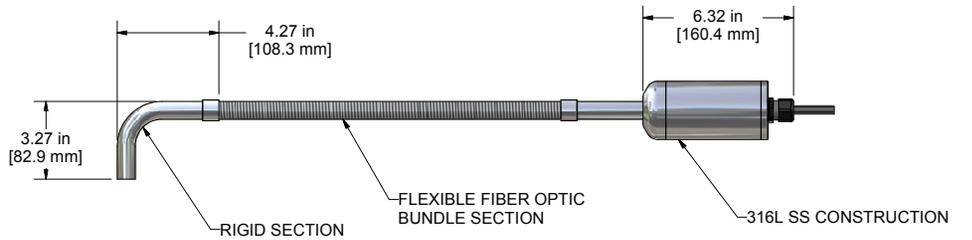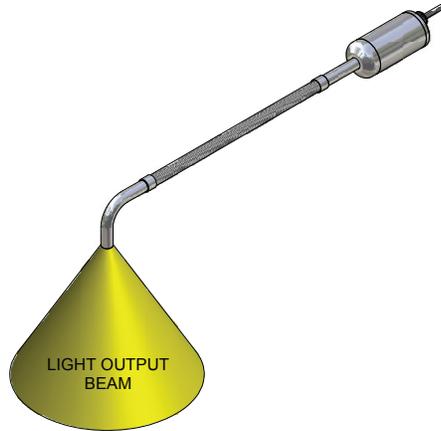

SIDE

MOUNT BUNDLE DIRECT TO SIGHTGLASS. FLEXIBLE FIBER OPTIC BUNDLE ALLOWS LIGHT TO BE MOUNTED REMOTELY. SEE DATASHEET TD10811-200 FOR OPTIONAL MOUNTING BRACKET OPTIONS.

### NOTES:

1. REFERENCE DATASHEET TA9683-1.

**NOTICE**  
 THIS DRAWING IS THE PROPERTY OF J.M. CANTY AND MUST BE RETURNED WITHOUT REPRODUCTION OR DUPLICATION, AT ANY TIME UPON REQUEST, BUT IN ANY EVENT AS SOON AS IT HAS SERVED THE PURPOSE FOR WHICH IT WAS FURNISHED, WHILE IN THE POSSESSION OF THE RECIPIENT, IT MUST BE PROPERLY SAFEGUARDED AGAINST DISCLOSURE TO ANYONE EXCEPT THOSE EMPLOYEES WHO REQUIRE IT FOR WORK OR JOB. THE RECIPIENT MUST KEEP CONFIDENTIAL AND REQUIRE HIS (HER) EMPLOYEES TO KEEP CONFIDENTIAL THE INFORMATION CONTAINED HERE ON.

**IMPORTANT**  
 FOR THE REQUIRED MANUFACTURING SPECIFICATIONS SEE DOCUMENT #A4955

**NOTE: FAILURE TO RECEIVE DOCUMENT DOES NOT WAIVE VENDOR RESPONSIBILITY**

|                                 |                   |
|---------------------------------|-------------------|
| DRAWN BY<br>JD                  | DATE<br>5/9/2007  |
| APPROVAL<br>JD                  | DATE<br>6/11/2007 |
| ENGINEERING ANALYSIS<br>CURRENT | DATE              |
| MFG. APPROVAL<br>PENDING        | DATE              |
| QUALITY CONTROL<br>I.O.A.       | DATE              |

|  |                                 |   |
|--|---------------------------------|---|
| J.M. CANTY INC.<br>6100 DONNER RD.<br>BUFFALO, N.Y. 14094<br>U.S.A.                        | <b>CANTY</b><br>WWW.JMCANTY.COM | J.M. CANTY INTL. LTD.<br>BALLYCOOLIN BUS. PK.<br>BLANCHARDSTOWN<br>DUBLIN 15, IRELAND |
| TITLE<br>HYL 52 LIGHT SYSTEM, EXTERNAL TRANSFORMER / PSU, FIBER OPTIC BUNDLE SPECIFICATION |                                 |   |
| SIZE / REVISION<br>C 0   | FILE NAME<br>TC9683-100         |   |
| SCALE AS NOTED   | SHEET 1 OF 1                    |   |

| SPECIFICATIONS        |  |
|-----------------------|--|
| MAX. TANK SIZE        | 8' [2.4m] $\varnothing$ X 12' [3.7m] DP.         |
| BULB                  | 50W HALOGEN. IDEAL WHITE LIGHT 3500°K            |
| INPUT VOLTAGE         | 12V AC 50/60 Hz OR DC FROM CANTY OR CUSTOMER PSU |
| TIMER                 | NOT REQ'D. MOMENTARY SERVICE ONLY                |
| MOMENTARY SWITCH      | AVAILABLE INTEGRAL OR EXTERNAL W/42" CORD        |
| INFRA-RED FILTER      | YES - REMOVES ALL HEAT. NO PRODUCT BAKE-ON       |
| ENVIRONMENTAL RATINGS | NEMA 4X, IP66                                    |