
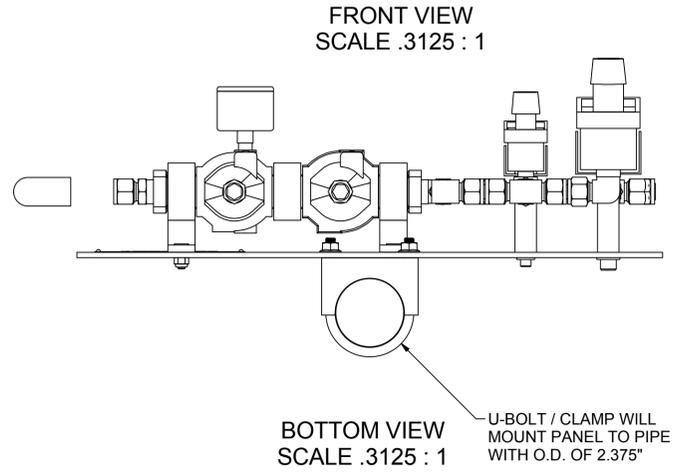
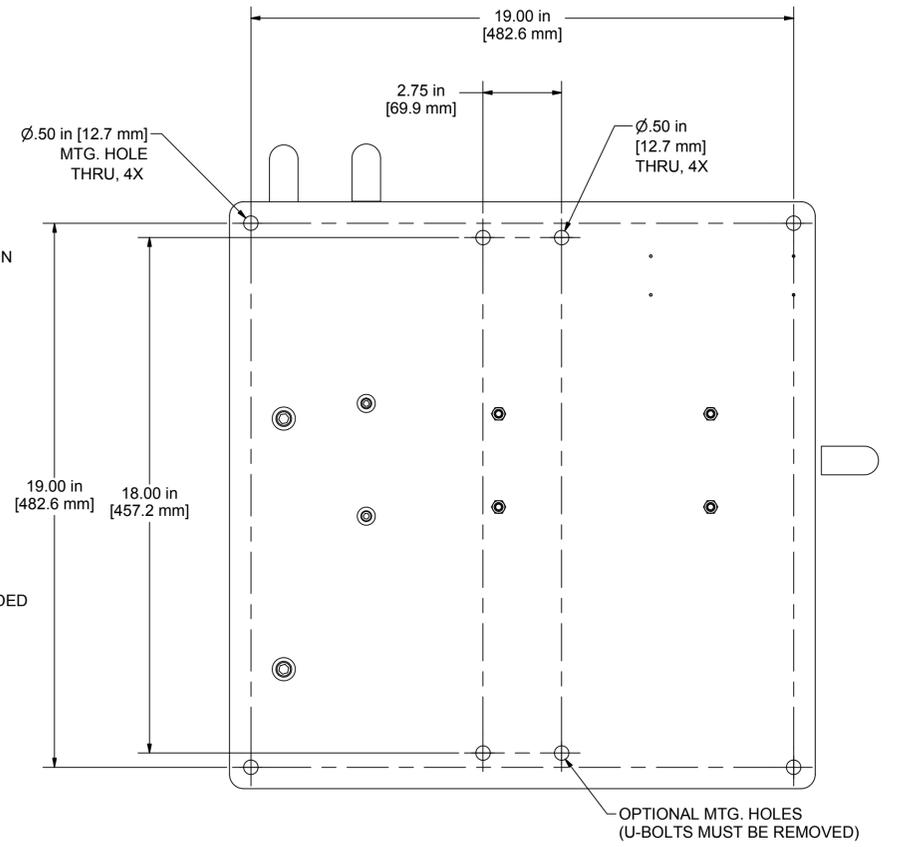
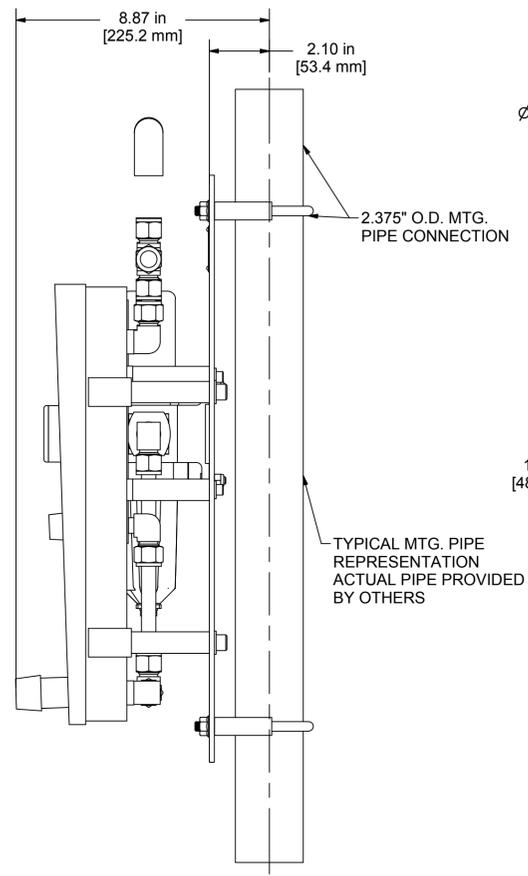
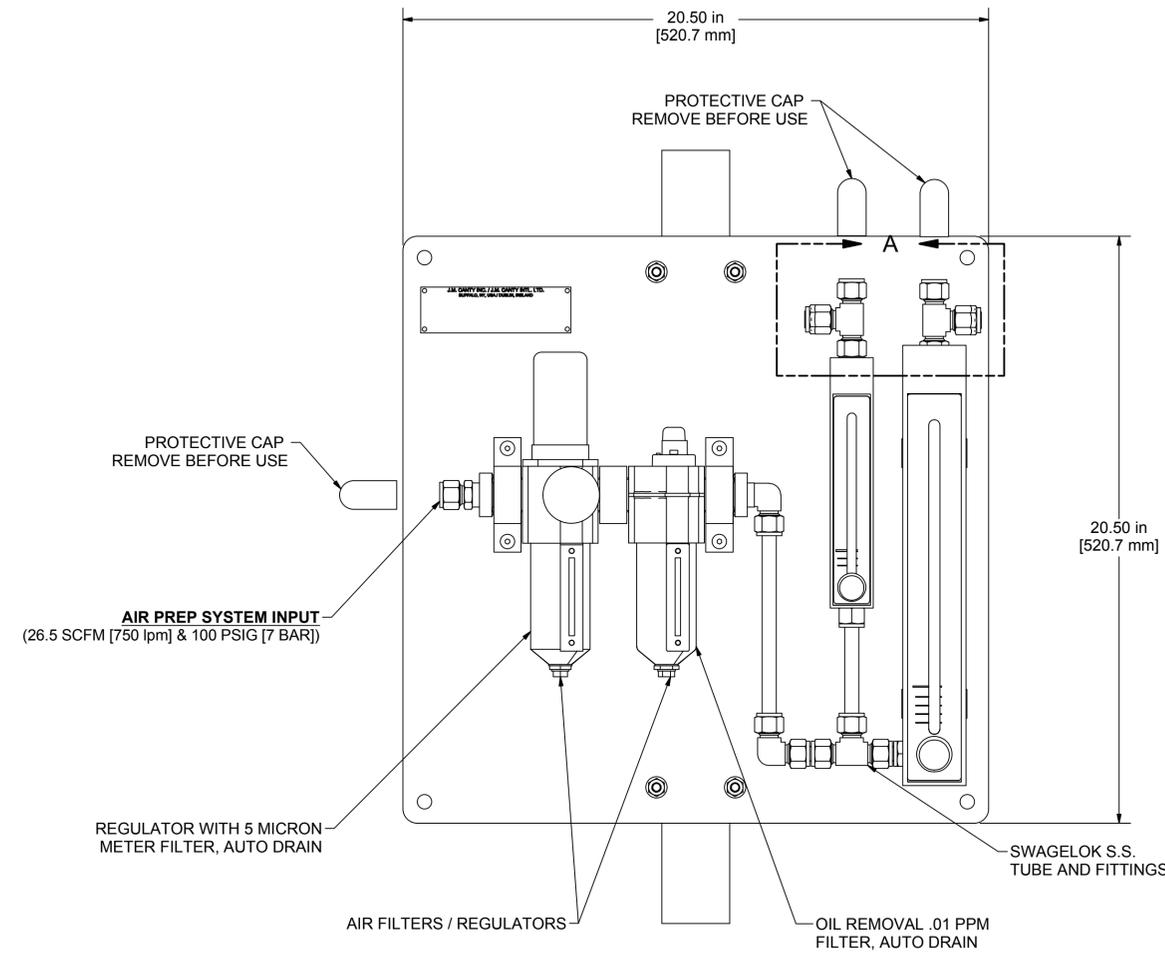


SPECIFICATIONS	
P/N	VC11415-190
MODEL	INST. AIR PREP. SYS, 1/2" TUBE, 2" PIPE MT., AL. PLATE
INPUT SPECIFICATIONS	CLEAN, DRY, MAX 100 PSIG [7 BAR], MAX TEMP. 125 F [51.6 C]
OUTPUT SPECIFICATIONS	AIR FILTERED TO .01 MICRON
FEATURES	
- CONSULT FACTORY REF DWG C11509-200 FOR HIGHER TEMPS	
- CLEAN DRY AIR MUST HAVE AT LEAST -20C DEWPOINT & NO OIL PRESENT	

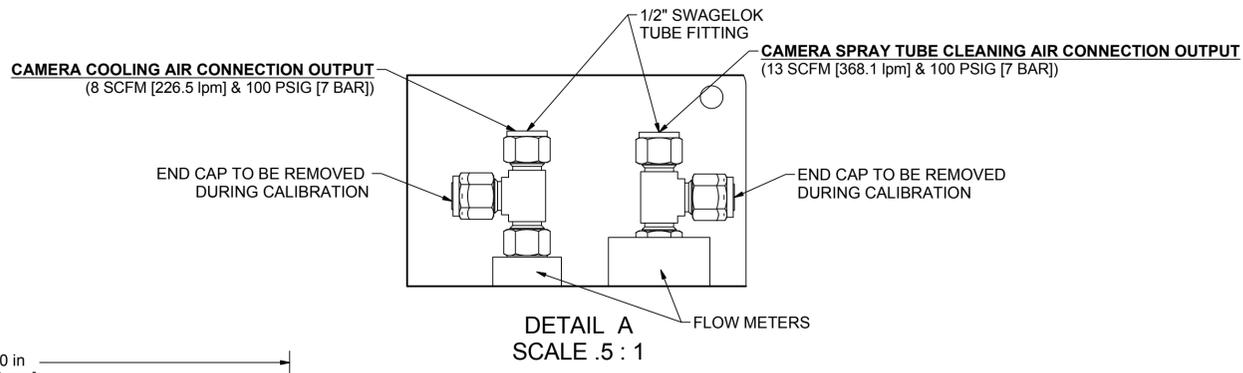

- NOTES:**
- AIR PREP SYSTEM INPUT REQUIREMENTS: 26.5 SCFM [750 lpm] & 100 PSIG [7 BAR].
 - APPROXIMATE WEIGHT : 27 LB. [12.2 KG].
 - ALL DIMENSIONS LISTED ARE THEORETICAL AND MAY VARY SLIGHTLY DUE TO MANUFACTURING TOLERANCES AND ASSEMBLY POSITION OF ADJUSTABLE PARTS.

NOTICE

THIS DRAWING IS THE PROPERTY OF J.M. CANTY AND MUST BE RETURNED WITHOUT REPRODUCTION OR DUPLICATION, AT ANY TIME UPON REQUEST, BUT IN ANY EVENT AS SOON AS IT HAS SERVED THE PURPOSE FOR WHICH IT WAS FURNISHED. WHILE IN THE POSSESSION OF THE RECIPIENT, IT MUST BE PROPERLY SAFEGUARDED AGAINST DISCLOSURE TO ANYONE EXCEPT THOSE EMPLOYEES WHO REQUIRE IT FOR WORK OR JOB. THE RECIPIENT MUST KEEP CONFIDENTIAL AND REQUIRE HIS (HER) EMPLOYEES TO KEEP CONFIDENTIAL THE INFORMATION CONTAINED HERE ON.

IMPORTANT FOR THE REQUIRED MANUFACTURING SPECIFICATIONS SEE DOCUMENT #A4955

NOTE: FAILURE TO RECEIVE DOCUMENT DOES NOT WAIVE VENDOR RESPONSIBILITY

DRAWN BY	MAC	DATE	25-Jan-16
APPROVAL	MAC	DATE	25-Jan-16
ENGINEERING ANALYSIS	CURRENT	DATE	
MFG. APPROVAL	PENDING	DATE	
QUALITY CONTROL	VJS	DATE	

J.M. CANTY INC. 6100 DONNER RD. BUFFALO, N.Y. 14094 U.S.A.		CANTY WWW.JMCANTY.COM		J.M. CANTY INTL. LTD. BALLYCOOLIN BUS. PK. BLANCHARDSTOWN DUBLIN 15, IRELAND	
TITLE INSTUMENT AIR PREP. SYS, 1/2" TUBE FOR H.T. VIS. SYS, 2" PIPE MT., AL. PLATE, VC11415-190					
REVISION	0	FILE NAME	TD11415-340		
SCALE	AS NOTED	SIZE	D	SHEET	1 OF 1