


IP66 AREA GENERAL PURPOSE AREA

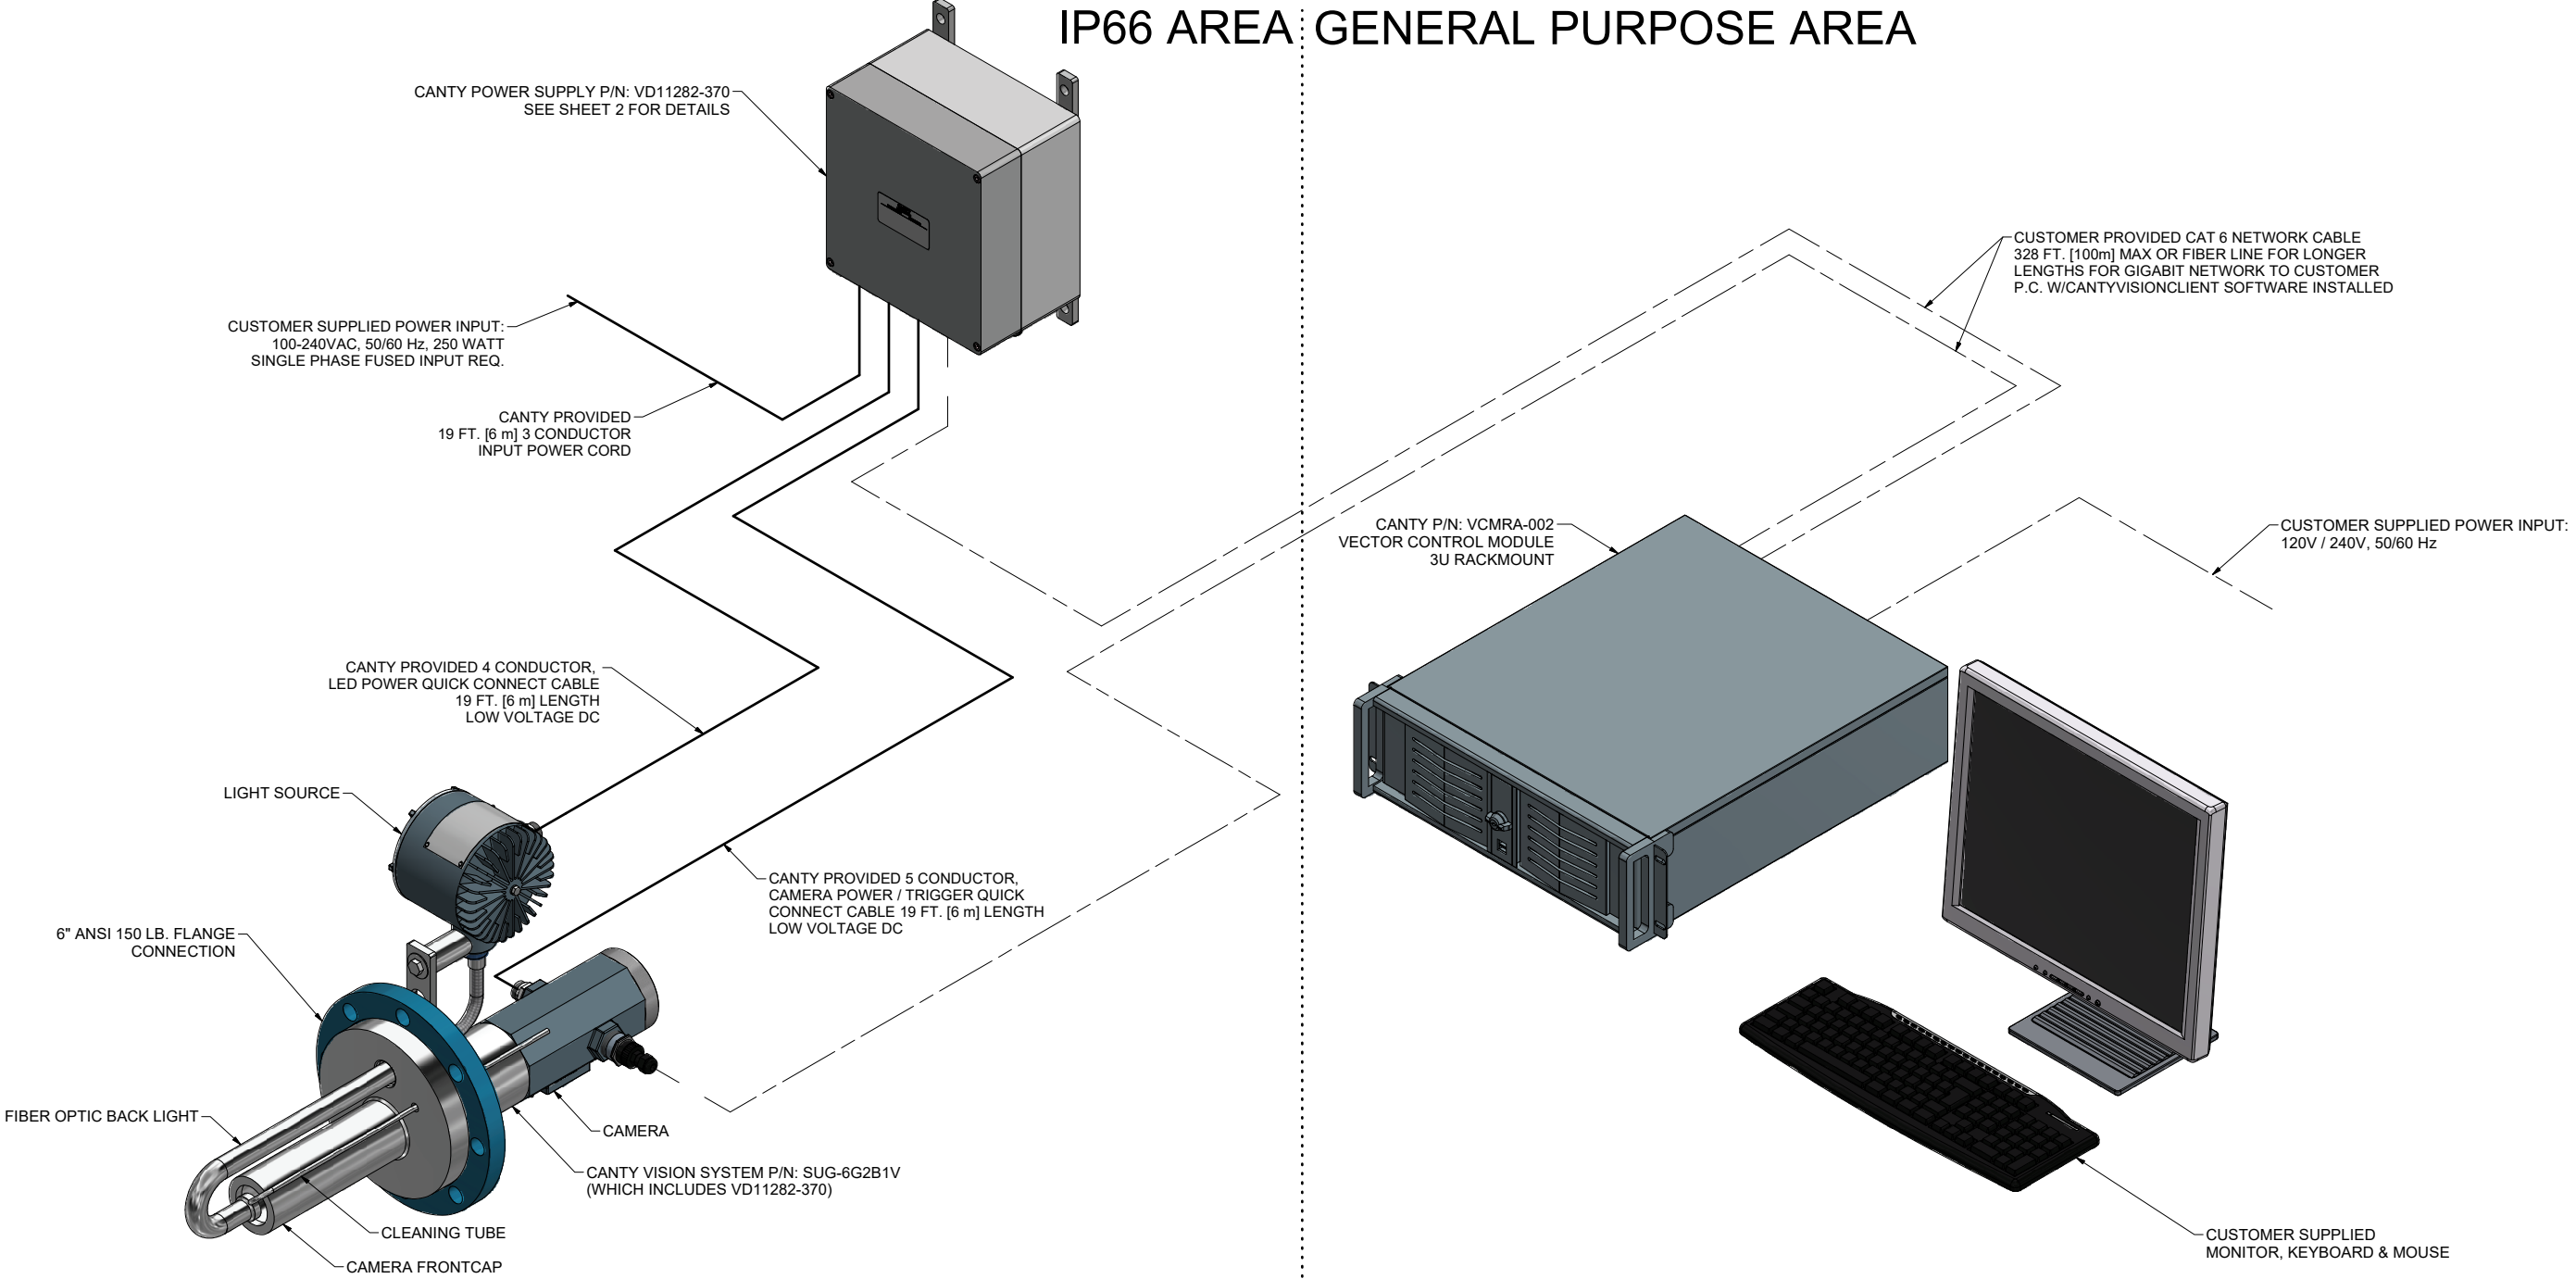


ISOMETRIC VIEW
SCALE .25 : 1


NOTES:

1. ALL WETTED METAL PARTS ARE ALLOY C276 & 316L S.S.. GLASS IS BOROPLUS. O-RING SEALS ARE VITON.
2. NON-WETTED PARTS ARE ALUMINUM WITH AN ANODIZED FINISH. ENCLOSURE O-RINGS ARE BUNA-N.
3. CAMERA AND LIGHT ARE RATED FOR USE IN IP66 LOCATIONS.
4. ALL WIRING & CONNECTORS SUPPLIED BY CUSTOMER MUST BE COMPLETED IN ACCORDANCE WITH APPLICABLE LOCAL AND PLANT REGULATIONS.
5. SYSTEM REQUIRES CUSTOMER SUPPLIED: 100-240VAC, 50/60 Hz, 250 WATT INPUT.
6. GIGABIT ETHERNET CAMERA HAS AN RJ-45 JACK, CUSTOMER SUPPLIES CAT6 CABLING WITH ENDS AS REQUIRED BETWEEN CAMERA AND VCM WITH CANTYVISION SOFTWARE INSTALLED.


NOTICE THIS DRAWING IS THE PROPERTY OF J.M. CANTY AND MUST BE RETURNED WITHOUT REPRODUCTION OR DUPLICATION, AT ANY TIME UPON REQUEST, BUT IN ANY EVENT AS SOON AS IT HAS SERVED THE PURPOSE FOR WHICH IT WAS FURNISHED. WHILE IN THE POSSESSION OF THE RECIPIENT, IT MUST BE PROPERLY SAFEGUARDED AGAINST DISCLOSURE TO ANYONE EXCEPT THOSE EMPLOYEES WHO REQUIRE IT FOR WORK OR JOB. THE RECIPIENT MUST KEEP CONFIDENTIAL AND REQUIRE HIS (HER) EMPLOYEES TO KEEP CONFIDENTIAL THE INFORMATION CONTAINED HERE ON.	IMPORTANT FOR THE REQUIRED MANUFACTURING SPECIFICATIONS SEE DOCUMENT #A4955 NOTE: FAILURE TO RECEIVE DOCUMENT DOES NOT WAIVE VENDOR RESPONSIBILITY	DRAWN BY RFM APPROVAL RFM ENGINEERING ANALYSIS CURRENT MFG. APPROVAL PENDING QUALITY CONTROL VJS	DATE 23-Sep-20 DATE 23-Sep-20 DATE DATE DATE	J.M. CANTY INC. 6100 DONNER BUS. PK. BUFFALO, N.Y. 14094 U.S.A. TITLE SUGAR SCOPE GENERAL ARRAIGNMENT DRAWING REVISION 0 FILE NAME VD11919-1146 SCALE AS NOTED SIZE D	CANTY WWW.JMCANTY.COM	J.M. CANTY INTL. LTD. BALLYCOOLIN BUS. PK. BLANCHARDSTOWN DUBLIN 15, IRELAND SHEET 1 OF 2
--	---	--	---	--	---	---

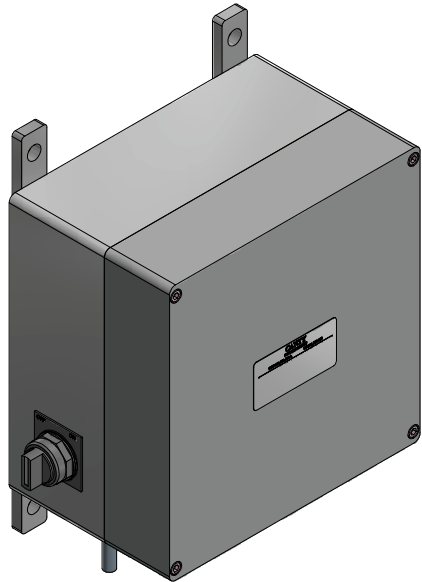


ISOMETRIC VIEW
SCALE .375 : 1

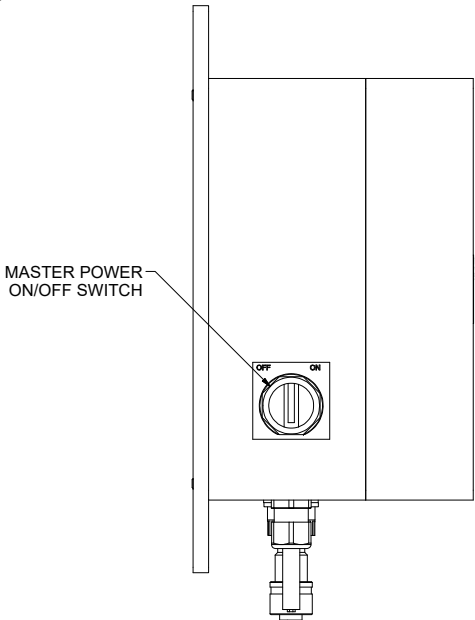

MASTER POWER
ON/OFF SWITCH

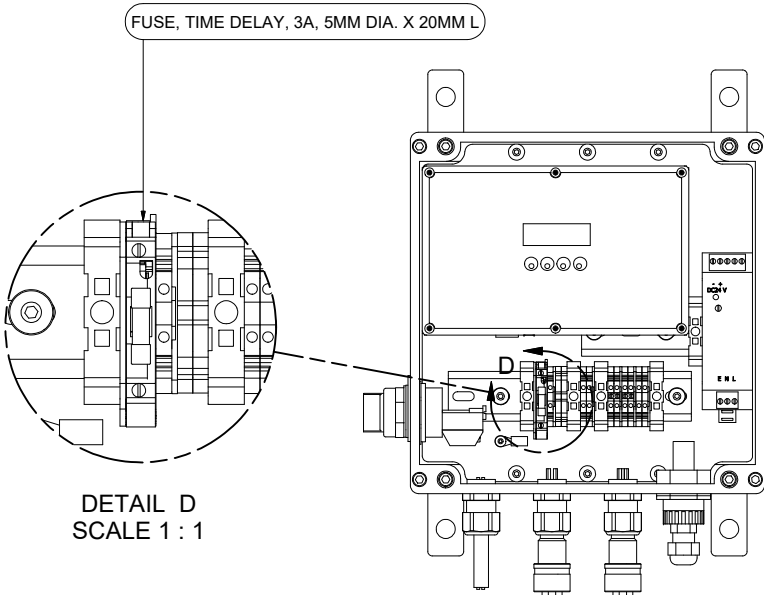

DETAIL D
SCALE 1 : 1

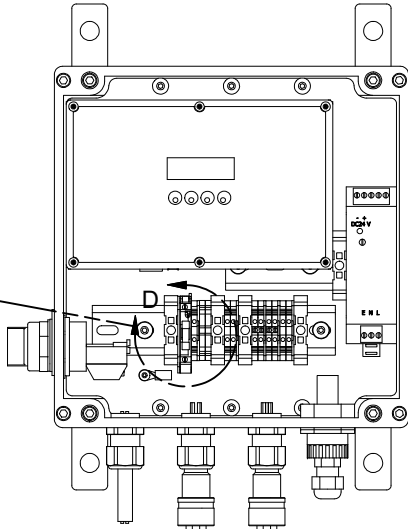

FRONT VIEW
SCALE .375 : 1
(COVER REMOVED)


WIRING DETAIL	
WIRE COLOR	FUNCTION
BROWN	LIVE INPUT
BLUE	NEUTRAL INPUT
GREEN	EARTH INPUT

POWER INPUT
3 CONDUCTOR WIRE, 19 ft. [6m]


RJ45 ATTACHABLE IP67
CABLE GLAND FOR
CAT 6 CABLE

5 PIN QUICK CONNECT CABLE
TO CAMERA HOUSING
19 ft. [6m] LENGTH



4 PIN QUICK CONNECT CABLE
TO LED HOUSING
19 ft. [6m] LENGTH

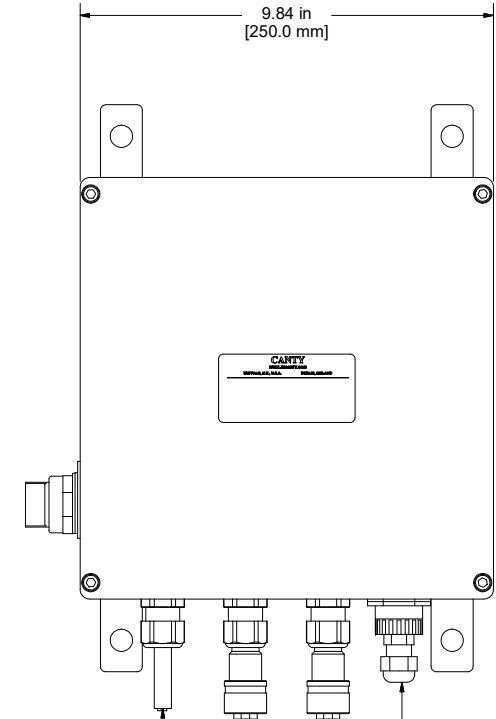

FRONT VIEW
SCALE .4375 : 1

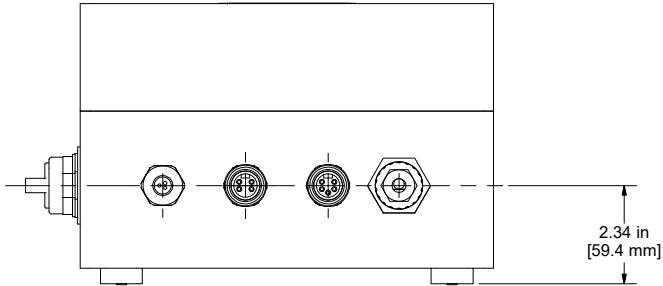

THIS SIDE UP

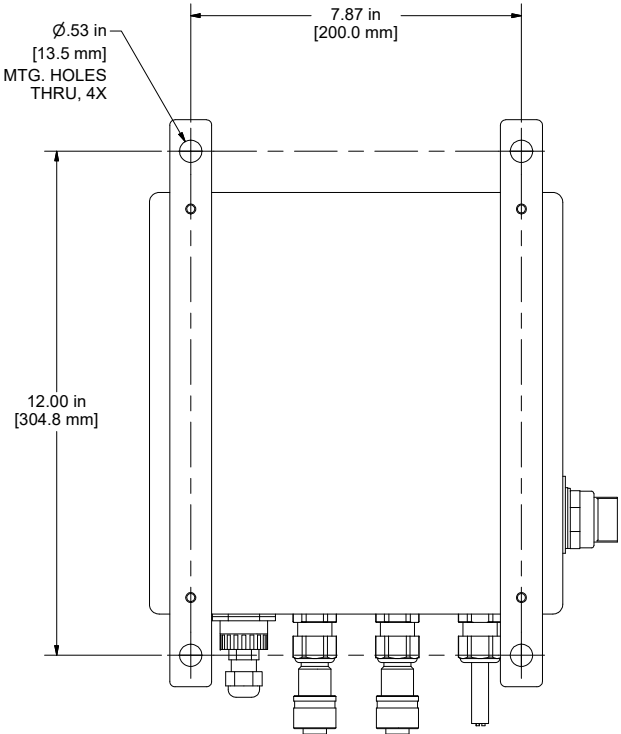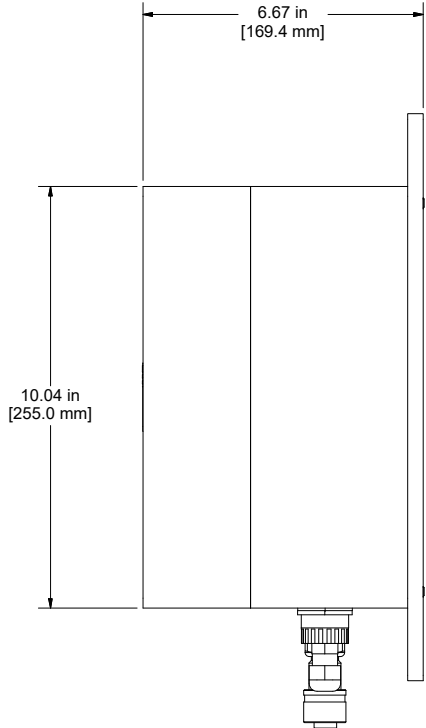

SPECIFICATIONS

P/N	VD11282-370
MODEL	PSU,WP/IP,REG.CAM./STRB.CTRL,POLY.ENCL.W/BKT.
INPUT SPECIFICATIONS	100-240VAC, 50/60 Hz, 250W SOURCE
OUTPUT SPECIFICATIONS	24VDC, 1A MAX.(CCD) : 50VDC, 3A MAX. (STROBE LED)

FEATURES

- WEATHER PROOF POWER SUPPLY NEMA TYPE 4X/IP66
- MAX RECOMMENDED CAT. 6 OUTPUT CABLE DISTANCE TO COMPUTER, 328 FT. [100 m] FOR STROBE CONTROL REMOTE CAPABILITIES.

NOTES:

1. ENCLOSURE MUST BE MOUNTED ON A PROPERLY SUPPORTED VERTICAL STRUCTURE IN THE ORIENTATION SHOWN.
2. APPROXIMATE WEIGHT: 14 LBS. [6.3 KGS].
3. ENCLOSURE DIMENSIONS AND ELECTRONIC COMPONENTS MAY VARY SLIGHTLY FROM WHAT IS SHOWN DUE TO MANUFACTURING IMPROVEMENTS. SYSTEM WILL STILL MAINTAIN THE SAME FORM AND FUNCTION AS INTENDED. SPECIFICATIONS SHOWN ARE CURRENT AT TIME OF APPROVAL DRAWING CREATION.

NOTICE
THIS DRAWING IS THE PROPERTY OF J.M. CANTY AND MUST BE RETURNED WITHOUT REPRODUCTION OR DUPLICATION, AT ANY TIME UPON REQUEST, BUT IN ANY EVENT AS SOON AS IT HAS SERVED THE PURPOSE FOR WHICH IT WAS FURNISHED. WHILE IN THE POSSESSION OF THE RECIPIENT, IT MUST BE PROPERLY SAFEGUARDED AGAINST DISCLOSURE TO ANYONE EXCEPT THOSE EMPLOYEES WHO REQUIRE IT FOR WORK OR JOB. THE RECIPIENT MUST KEEP CONFIDENTIAL AND REQUIRE HIS (HER) EMPLOYEES TO KEEP CONFIDENTIAL THE INFORMATION CONTAINED HERE ON.

IMPORTANT
FOR THE REQUIRED
MANUFACTURING
SPECIFICATIONS SEE
DOCUMENT #A4955

NOTE: FAILURE TO
RECEIVE DOCUMENT
DOES NOT WAIVE
VENDOR
RESPONSIBILITY

DRAWN BY RFM	DATE 23-Sep-20	J.M. CANTY INC. 6100 DONNER RD. BUFFALO, N.Y. 14094 U.S.A.		CANTY WWW.JMCANTY.COM		J.M. CANTY INTL. LTD. BALLYCOOLIN BUS. PI BLANCHARDSTOWN DUBLIN 15, IRELAND	
APPROVAL RFM	DATE 23-Sep-20	TITLE SUGAR SCOPE GENERAL ARRAIGNMENT DRAWING					
ENGINEERING ANALYSIS CURRENT	DATE						
MFG. APPROVAL PENDING	DATE						
QUALITY CONTROL VJS	DATE						
		REVISION 0		FILE NAME VD11919-1146			
		SCALE AS NOTED		SIZE D		SHEET 2 OF 2	